

Open-top Bessel beam two-photon light sheet microscopy for three-dimensional pathology

Reviewed Preprint

Published from the original preprint after peer review and assessment by eLife.

About eLife's process

Reviewed preprint posted

November 30, 2023 (this version)

Posted to bioRxiv

October 20, 2023

Sent for peer review

October 2, 2023

Won Yeong Park, Jieun Yun, Jinho Shin, Byung Ho Oh, Gilsuk Yoon, Seung-Mo Hong, Ki Hean Kim 

Department of Mechanical Engineering, Pohang University of Science and Technology, Pohang, Gyeongsangbuk, 37673, Republic of Korea • Department of Medicine, University of Ulsan College of Medicine, Seoul, 05505, Republic of Korea • Department of Dermatology, College of Medicine, Yonsei University, Seoul, 03722, Republic of Korea • Department of Pathology, School of Medicine, Kyungpook National University, Daegu, 41944, Republic of Korea • Department of Pathology, Asan Medical Center, University of Ulsan College of Medicine, Seoul, 05505, Republic of Korea • Department of I-Bio, Pohang University of Science and Technology, Pohang, Gyeongsangbuk, 37673, Republic of Korea

 https://en.wikipedia.org/wiki/Open_access

 Copyright information

Abstract

Nondestructive pathology based on three-dimensional (3D) optical microscopy holds promise as a complement to traditional destructive hematoxylin and eosin (H&E) stained slide-based pathology by providing cellular information in high throughput manner. However, conventional techniques provided superficial information only due to shallow imaging depth. Herein, we developed open-top two-photon light sheet microscopy (OT-TP-LSM) for intraoperative 3D pathology. An extended depth of field two-photon excitation light sheet was generated by scanning a nondiffractive Bessel beam, and selective planar imaging was conducted with cameras at 400 frames/s max during the lateral translation of tissue specimens. Intrinsic second harmonic generation was collected for additional extracellular matrix (ECM) visualization. OT-TP-LSM was tested in various human cancer specimens including skin, pancreas, and prostate. High imaging depths were achieved owing to long excitation wavelengths and long wavelength fluorophores. 3D visualization of both cells and ECM enhanced the ability of cancer detection. Furthermore, an unsupervised deep learning network was employed for the style transfer of OT-TP-LSM images to virtual H&E images. The virtual H&E images exhibited comparable histological characteristics to real ones. OT-TP-LSM may have the potential for histopathological examination in surgical and biopsy applications by rapidly providing 3D information.

eLife assessment

This **important** work by Park et al. introduces an open-top two-photon light sheet microscopy (OT-TP-LSM) for lesser invasive evaluation of intraoperative 3D pathology. The authors provide **convincing** evidence for the effectiveness of this technique in investigating various human cancer cells. The paper needs some minor corrections and has the potential to be of broad interest to biologists and, specifically, pathologists utilizing 3D optical microscopy.

Introduction

Conventional histopathological examination using thin sectioning and hematoxylin and eosin (H&E) staining has inherent limitations, including long processing time, tissue loss, sampling error, limited two-dimensional (2D) information, and artifacts. High-speed three-dimensional (3D) optical microscopy, which can visualize cellular structures without thin sectioning, holds promise for nondestructive 3D pathological examination [1–4]. Various high-speed 3D microscopy techniques have been developed [5–12], and open-top light sheet microscopy (OT-LSM) is a promising technique that enables high-throughput imaging with sheet illumination and planar imaging on uneven tissue surfaces [13–16]. OT-LSM is a specialized form of LSM for imaging large tissue specimens such as biopsy specimens by placing all the optical components below the sample holder. However, fluorescence 3D microscopy techniques, including OT-LSM, have shallow imaging depths in turbid tissue owing to high excitation light scattering and absorption, which limits precise 3D histopathology. As alternative method for high depth imaging, two-photon microscopy (TPM) has been used [17–19]. TPM is based on nonlinear excitation of fluorophores and achieves high imaging depths up to a few hundred micrometers by using long excitation wavelengths, which reduce light scattering. Furthermore, TPM provides additional intrinsic second harmonic generation (SHG) contrast for imaging collagen in the extracellular matrix (ECM) [20–22]. Two-photon LSM (TP-LSM) techniques have been developed for high-speed and high-depth imaging of live small animals and biological studies [23–27], but they were not in an open-top configuration.

In this study, we present the development of an open-top TP-LSM (OT-TP-LSM) with a Bessel beam for high-throughput and high-depth 3D pathological examination of large biopsied tissue specimens. A nondiffractive Bessel beam was used for the generation of an extended depth of field (EDOF) excitation light sheet with minimal side lobe effects [28, 29]. High imaging depths were achieved by using long excitation wavelengths and fluorescent nuclear probes emitting relatively long wavelengths. After development and characterization, the system was applied to high-throughput 3D imaging of various human cancer specimens, including skin, pancreas, and prostate in comparison with conventional H&E stained images for verification. Moreover, OT-TP-LSM images were converted to virtual H&E images using deep learning style transfer. We demonstrate that OT-TP-LSM imaging is comparable to that obtained from H&E stained slides for several human cancer types and has the potential for rapid and accurate nondestructive 3D pathology.

Results

Open-top two-photon light sheet microscopy (OT-TP-LSM) for 3D pathology

Schematics and characterization results of OT-TP-LSM are presented in **Figure 1**. OT-TP-LSM is an orthogonally arranged dual objective LSM with a liquid prism interface (**Figure 1A**). All optical components of OT-TP-LSM were positioned underneath a sample holder to accommodate large size specimens without physical interference with the illumination and imaging optics. Two 20x air objective lenses with a moderate numerical aperture (NA) of 0.42 were used to deliver a thin excitation light sheet and collect emission light efficiently. The custom liquid prism was used to transmit excitation light into the specimen and to collect emission light out with minimal aberration by refractive index (RI) matching with different mediums where the sample was immersed (**Figure 1B**). The liquid prism was filled with diluted glycerol in distilled water, whose RI was matched to that of a quartz (RI: 1.45) window in a sample holder. A Ti:Sapphire laser

beam was expanded and converted to a Bessel beam using an axicon lens. The Bessel beam was reflected on a galvanometer scanner and relayed to the sample through the liquid prism by a combination of a tube lens and an objective lens. The scanner scanned the Bessel beam to form an EDOF excitation light sheet. Emission light generated by the sample was collected by the imaging objective lens through the liquid prism, split into two channels, one for fluorescence and the other for SHG, using a dichroic mirror, and imaged simultaneously by two scientific complementary metal-oxide– semiconductor (sCMOS) cameras with individual gain control.

The excitation light sheet was designed to have a DOF of 180 μm with a thickness of 0.9 μm (**Figure 1 - figure supplement 1** [↗](#)). The imaging field of view was 600 $\mu\text{m} \times 170 \mu\text{m}$ with 2,048 $\times$ 512 pixels and was limited by the DOF of the Bessel beam. Emission light scattering in the specimen further limited the imaging depth. Selective planar images along the oblique excitation light sheet were acquired sequentially with a stepwise X-axis translation of the specimen by the motorized stage (**Figure 1C** [↗](#)). A graphical user interface based on LabVIEW was used to generate trigger signals for both the cameras and the motorized stage. OT-TP-LSM was characterized by imaging fluorescent microspheres (0.5 μm in diameter) embedded in agarose gel, whose RI was matched to that of the solution in the liquid prism (**Figure 1D** [↗](#)). The image throughput was 0.24 mm^2/s at an acquisition rate of 400 fps and step size of 1 μm . The image resolution was measured to be 0.9 μm in all dimensions. The lateral resolution in the Y-Z' plane was approximately 128% of the theoretical value due to spherical aberration induced by the RI mismatch between air and the immersion medium, but this was sufficient for detecting cellular features.

The imaging depth of OT-TP-LSM was evaluated using freshly excised human skin specimens. Proflavine was topically instilled onto the specimen for nuclear labeling before imaging. A representative Y-Z' plane image is shown in **Figure 1E** [↗](#). The imaging depth in the skin was approximately 90 μm in the 45°-tilted image plane, and the actual depth was 64 μm from the surface. To compare the imaging depth, the same skin specimen was imaged using conventional one-photon excitation-based LSM (1PLSM). The imaging depth was approximately 28 μm in the 45°-tilted image plane and 20 μm from the surface, which was approximately three times less than that of OT-TP-LSM. While the imaging depth of OT-TP-LSM was sufficient for visualizing 3D cell structures in the skin, it was relatively low compared to that of conventional point-scanning based TPM due to the effect of emission photon scattering.

3D OT-TP-LSM imaging of human skin cancers

After development and characterization, the performance of OT-TP-LSM was assessed in human skin cancer specimens. Representative OT-TP-LSM images of two basal cell carcinoma (BCC) specimens are presented along with H&E stained histology images in **Figure 2** [↗](#). The H&E images were obtained from the same specimens at slightly different depths. The OT-TP-LSM images visualized both cell structures and ECM in the cross-sectioned skin specimens, where proflavine-labeled cell nuclei and SHG-emitting collagen were depicted in green and blue, respectively. A mosaic image of the first BCC specimen visualized the epidermis as a thin layer on the top and the underlying dermis, most of which was occupied by BCC nests (**Figure 2A** [↗](#)). The epidermis and dermis were easily identifiable with SHG contrasts. Two regions of interest (ROI) were selected in the epidermis and BCC, and magnified images of these ROIs are presented to show the detailed cell structures. Magnified image in the epidermis (ROI 1) showed layered squamous epithelial cells (**Figure 2B** [↗](#)). Squamous cells in the basal layer were relatively large and individually resolved, while those in the upper layers were unresolved with relatively small cytoplasm and appeared as a band. Magnified images of BCC (ROI 2) showed many irregularly shaped tumor nests composed of densely packed monomorphic tumor cells of the same size (**Figure 2C** [↗](#)).

The mosaic image of the second BCC specimen mainly showed two different cell structures in the dermis (**Figure 2D** [↗](#)). The structures on the right side were BCCs, while those on the left side had intact ECM composition and differed from BCCs. The corresponding H&E stained histology image confirmed these as BCCs and normal gland structures in the dermis, respectively. Two ROIs were

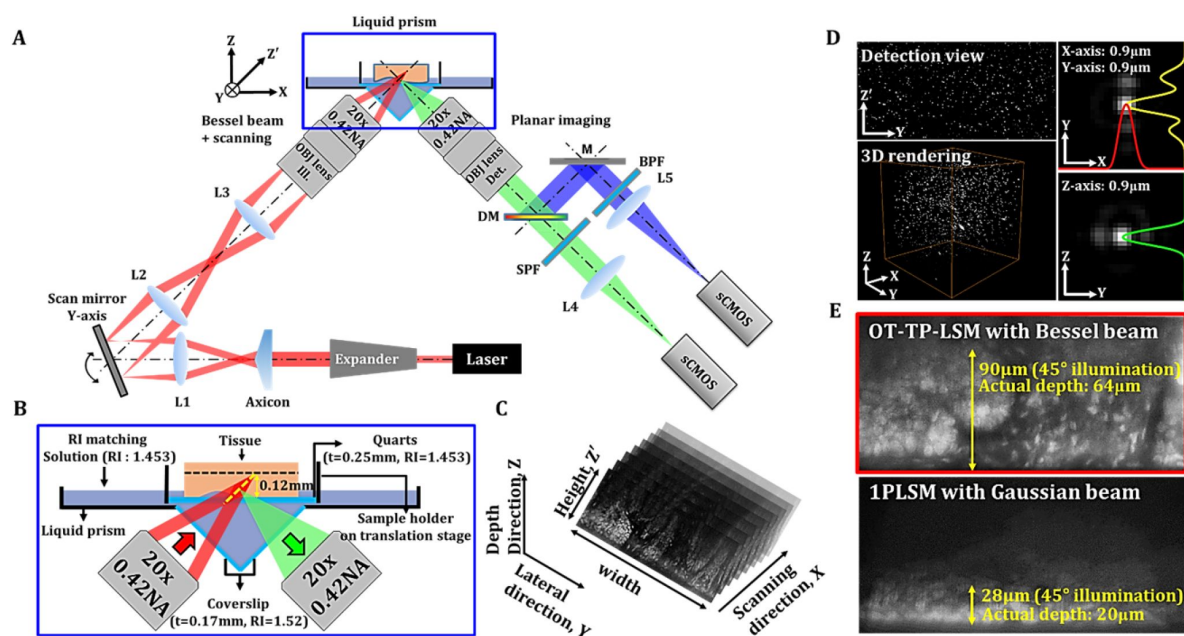


Figure 1.

Schematics and characteristics of open-top two-photon light sheet microscopy (OT-TP-LSM)

(A) Overall design of OP-TP-LSM. L: lens; M: mirror; DM: dichroic mirror; SPF: short pass filter; BPF: band pass filter; OBJ: objective lens. (B) Detailed schematic of the sample interface, including the liquid prism filled with refractive index (RI)-matching solution. (C) Illustration of sequential light sheet imaging with stepwise lateral translation. (D) Image resolution characterized by three-dimensional (3D) imaging of $0.5\ \mu\text{m}$ fluorescent microspheres. (E) Imaging depth characterized by imaging a proflavine-labeled fresh human skin specimen in comparison with that of one-photon light sheet microscopy (1PLSM) using Gaussian excitation sheet.

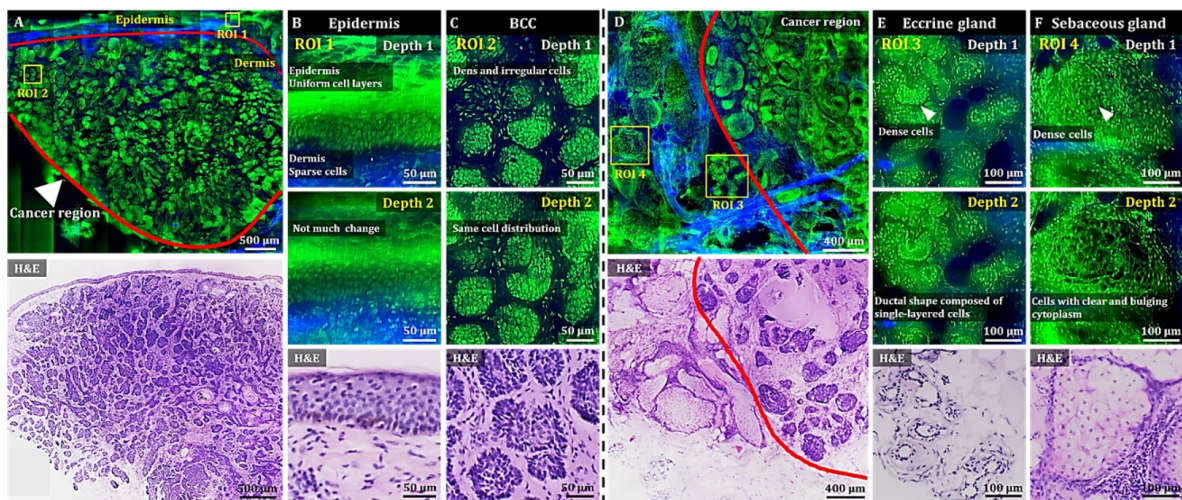


Figure 2.

3D OT-TP-LSM images of fresh human skin cancer (basal cell carcinoma, BCC) specimens

(A) Large-sectional OT-TP-LSM and hematoxylin and eosin (H&E) stained slide images of a BCC case 1. (B and C) Two magnified images of regions of interest (ROIs) with corresponding H&E images. ROI 1 and 2 were in the epidermis and superficial dermis and the BCC region below, respectively. (D) Large-sectional OT-TP-LSM and H&E images of a BCC case 2. (E and F) Two magnified images of ROIs with corresponding H&E images. ROI 3 and 4 were in eccrine and sebaceous glands, respectively. Superficial cell layers of both glands are marked with a white arrow. In the OT-TP-LSM images, proflavine fluorescence and second harmonic generation (SHG) are displayed in green and blue, respectively.

selected in the nontumorous skin region, and magnified images at two different depths are presented along with their corresponding H&E stained images. Magnified images of ROI 3 visualized clusters of small round tubular structures (**Figure 2E** [↗](#)). The image at depth 2 showed a duct structure composed of single-layered cuboidal epithelial cells, which is typical of eccrine glands. Magnified images of ROI 4 at two different depths showed pear-shaped clusters consisting of cells with clear and bulging cytoplasm, which is typical of sebaceous glands (**Figure 2F** [↗](#)). Using 3D visualization, normal glandular structures in the dermis were distinguished from BCC tumor nests (Video 1). Both eccrine and sebaceous glands could appear similar to BCC nests in 2D images at certain depths. Hence, 3D visualization would be important for distinguishing them.

3D OT-TP-LSM imaging of human pancreatic cancers

We then used OT-TP-LSM to visualize human pancreas specimens including those with pancreatic cancer. Instead of proflavine, propidium iodide (PI) was used as a nuclear labeling agent to increase the imaging depth (**Figure 3 - figure supplement 1** [↗](#)). The proflavine-labeled pancreas specimens had a relatively shallow imaging depth (up to 30 μm approximately) owing to the dense desmoplastic stromal cell composition. PI labeling allowed for deeper imaging up to approximately 55 μm from the surface due to the longer peak emission wavelength of 640 nm compared to proflavine. PI cytoplasmic labeling also occurred in addition to nuclear labeling of both acinar and neoplastic cells, probably owing to PI labeling of both DNA and RNA (**Figure 3 - figure supplement 2** [↗](#)) [[30](#) [↗](#), [31](#) [↗](#)]. Cell nuclei were identified with relatively strong fluorescence in the membrane and weaker fluorescence in the core. Representative OT-TP-LSM images and corresponding H&E stained slide images of normal pancreas and premalignant lesion specimens, and a pancreatic cancer (also known as pancreatic ductal adenocarcinoma, PDAC) specimen are shown in **Figures 3** [↗](#) and **4** [↗](#), respectively. The mosaic image of the normal pancreas visualized a dense distribution of acini composed of exocrine acinar cells in good correlation with the corresponding H&E image (**Figure 3A** [↗](#)). Two ROIs were selected, and magnified images are presented to show detailed cytologic features of the normal pancreas. Magnified images of ROI 1 visualized the cellular structure of acini and islets of Langerhans expressing different fluorescence intensities (**Figure 3B** [↗](#)). Acini were composed of lobules of acinar cells, and the boundaries of the acini were identified with relatively low PI fluorescence. The islets of Langerhans expressed relatively low PI fluorescence, probably due to the high composition of crystallized insulin in beta cells [[32](#) [↗](#)]. Magnified images of ROI 2 visualized a duct in the normal pancreas (**Figure 3C** [↗](#)). The duct was composed of single-layered cuboidal epithelial cells with round nuclei and was surrounded by dense fibrous tissue expressing SHG. The mosaic image of the pancreatic premalignant lesion exhibited different and irregular structures, including dilated ducts with intraductal proliferation of papillary structures (**Figure 3D** [↗](#)). Two different types of precursor lesions, intraductal papillary mucinous neoplasm (IPMN) and pancreatic intraepithelial neoplasia (PanIN), were observed [[33](#) [↗](#), [34](#) [↗](#)], and tumor cells were tall columnar containing intracytoplasmic mucin [[35](#) [↗](#)]. A corresponding H&E histology image confirmed the precursor lesions. Magnified images of PanIN (ROI 3) at two different depths showed proliferation of papillary epithelial cells with intracytoplasmic mucin, and 3D morphology of the PanIN (**Figure 3E** [↗](#)). OT-TP-LSM images were very similar to the corresponding H&E images, indicating OT-TP-LSM provided comparable histopathological information to that of H&E stained slides without thin sectioning.

A mosaic image of the PDAC arising from the IPMN specimen showed various abnormal ductal structures including cancer glands, IPMN, and surrounding pancreatitis, which were confirmed by the corresponding H&E stained slide image (**Figure 4A** [↗](#)). More desmoplastic fibrous stroma and a few abnormal cancer glands were observed compared to normal pancreas tissue [[36](#) [↗](#), [37](#) [↗](#)]. Two ROIs were selected in the PDAC region and the boundary region with nonneoplastic pancreatitis, and magnified images are presented to show detailed cellular structures. Magnified images of ROI 1 (PDAC) at two different depths showed irregularly shaped glands with sharp angles (**Figure 4B** [↗](#)). The glands exhibited disorganized cancer cell arrangement with nuclear membrane distortion. Magnified images of ROI 2 showed both nonneoplastic ducts and cancer

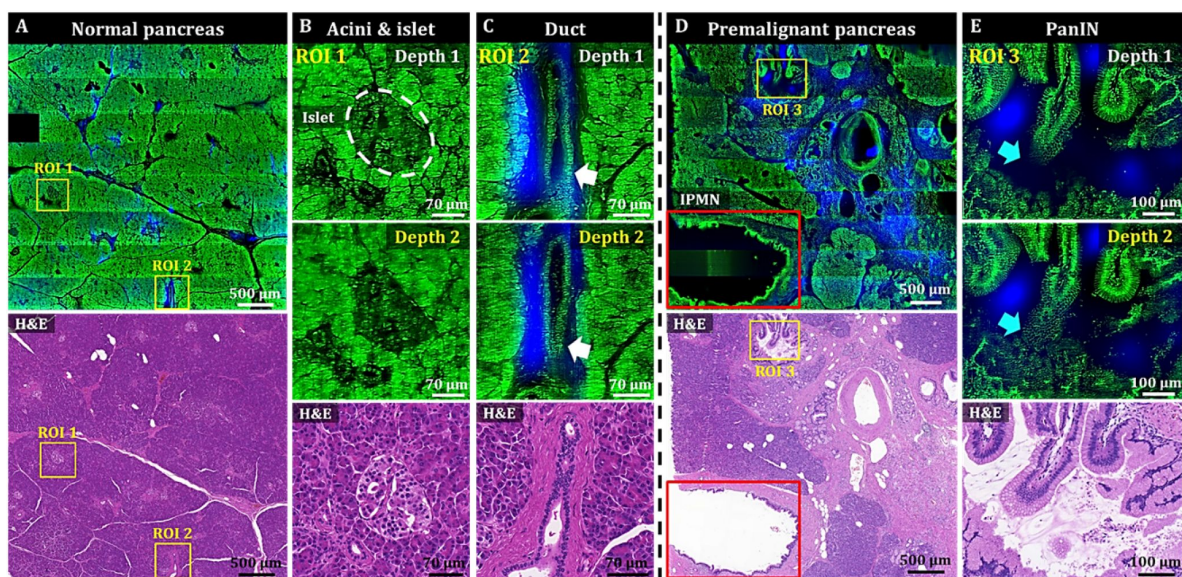


Figure 3.

3D OT-TP-LSM images of two human pancreas specimens: normal and premalignant lesion

(A) Large-area OT-TP-LSM and H&E stained images of normal human pancreas. (B and C) Magnified two-depth OT-TP-LSM images of ROI 1 and 2 in the normal pancreas and the corresponding H&E stained slide images. ROI 1 and 2 were on the acini and islets of Langerhans and the pancreatic duct, respectively. 3D morphological change of the duct was marked with a white arrow. (D) Large-area OT-TP-LSM and H&E stained images of a pancreatic premalignant lesion. Red box indicates the intraductal papillary mucinous neoplasm (IPMN). (E) Magnified two-depth OT-TP-LSM images of ROI 3 and corresponding H&E image of pancreatic intraepithelial neoplasia (PanIN). 3D morphological change of papillary in the PanIN was marked with a cyan arrow. In OT-TP-LSM images, propidium iodide (PI)-labeled cells and SHG-emitting collagen are displayed in green and blue, respectively.

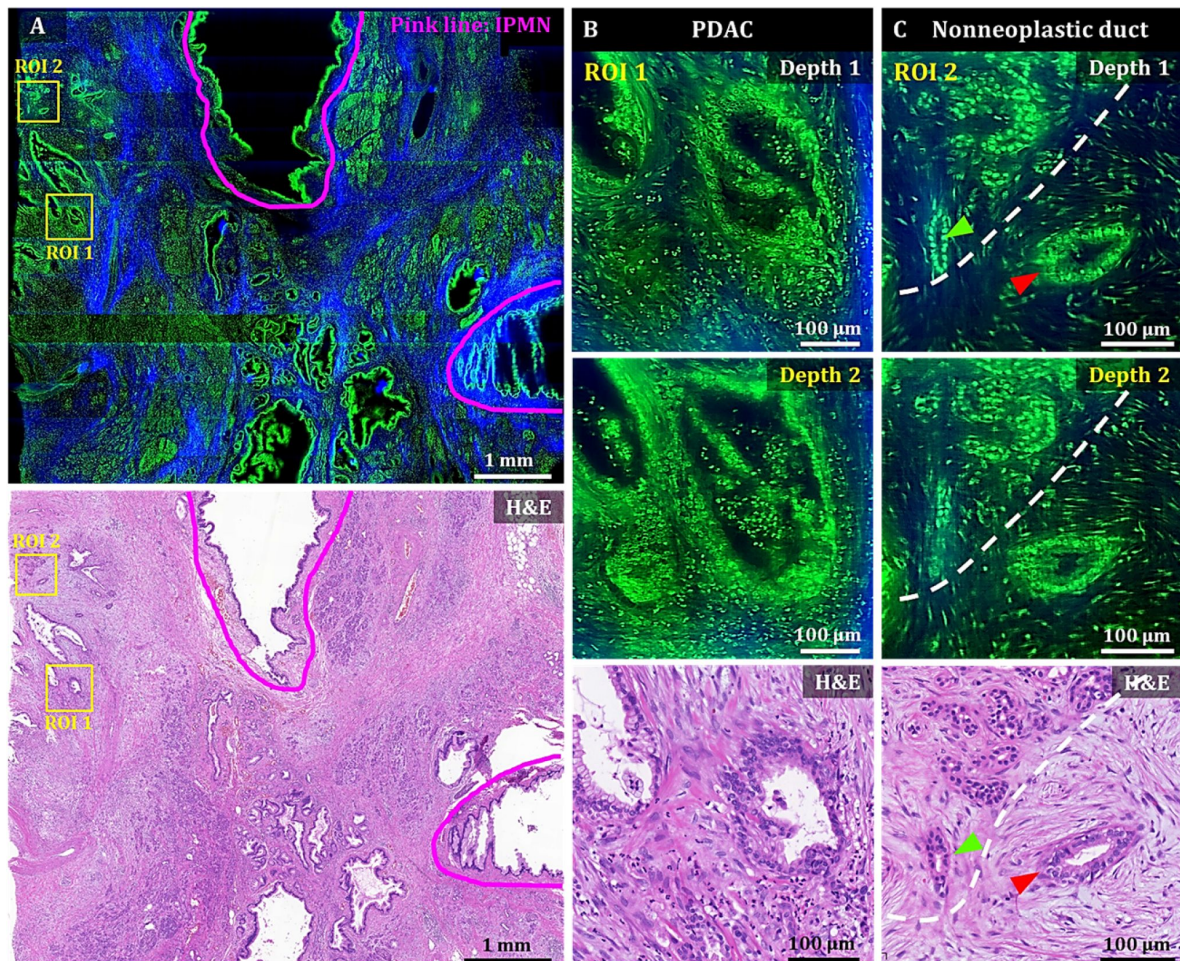


Figure 4.

3D OT-TP-LSM images of human pancreatic ductal adenocarcinoma (PDAC)

(A) Large-area OT-TP-LSM and H&E stained slide images of PDAC arising from IPMN specimen. Pink solid line indicates the IPMN area. (B and C) Magnified two-depth OT-TP-LSM images of ROI 1 and 2 in the PDAC region and the corresponding H&E stained images. ROI 1 was on the PDAC, and ROI 2 was on the boundary region between nonneoplastic pancreatitis and PDAC, respectively. A nonneoplastic duct and a PDAC were marked with green and red arrows, respectively. A white dashed line indicated the boundary between nonneoplastic pancreatitis and PDAC. In the OT-TP-LSM images, PI-labeled cells and SHG-emitting collagen are displayed in green and blue, respectively.

glands in different cell arrangements (**Figure 4C**). The nonneoplastic ducts had small, evenly distributed cells with relatively high nuclear fluorescence. Cancer glands, on the other hand, had disorganized and multilayered nuclei.

3D OT-TP-LSM imaging of human prostatic cancers

OT-TP-LSM was used to visualize human prostatectomy specimens, and two representative OT-TP-LSM images of benign and adenocarcinoma specimens are presented in **Figure 5**. The mosaic image of the histologically confirmed benign prostate showed benign glands dispersed throughout the specimen with relatively weak SHG composition between the glands (**Figure 5A**). An ROI was selected on benign glands, and magnified images are presented to show cytologic features alongside the corresponding H&E stained slide image (**Figure 5B**). Multiple cell layers, consisting of secretory cells and basal cells, lined the central lumen in the ducts of benign glands. Although images at two different depths are presented, the cell distribution was similar because of the relatively small depth difference compared to the gland size. The mosaic image of the prostate adenocarcinoma in **Figure 5C** showed both the benign and cancer regions, whose boundary was marked with a white solid line, and they were confirmed by the corresponding H&E stained image. The cancer region was full of crowded small gland structures, whereas the benign region consisted of relatively large glands surrounded by fibrous stroma. Magnified images of ROI 2 in the cancer region showed small glands composed of monolayered cell walls (**Figure 5D**). The cancer glands had single-layered malignant secretory cells only due to the loss of basal cell layers. The corresponding H&E histology was diagnosed as Gleason score 3+3 prostatic adenocarcinoma. OT-TP-LSM provided histological information equivalent to that of the H&E stained image without the need for sectioning.

Deep learning-based style transfer for virtual H&E

OT-TP-LSM images visualized histological features with high similarity to those in H&E images, but they may be unfamiliar to pathologists and clinicians accustomed to traditional H&E stained slide histology. PI-labeled OT-TP-LSM images were converted to virtual H&E images using Cycle-consistent generative adversarial network (CycleGAN) [38]. Representative virtual H&E images of pancreatic premalignant (PanIN) and PDAC are presented along with the corresponding real H&E stained images for comparison in **Figure 6**. Mosaic virtual H&E images of both PanIN and PDAC showed similar patterns to the corresponding real H&E stained histology images (**Figure 6A, C**). Although the normal region in the lower left corner of the virtual PanIN image was not transformed properly possibly due to insufficient image data of normal acini for training (**Figure 6A**), the magnified virtual H&E images clearly displayed distinct cell distributions of PanIN and PDAC by labeling cell cytoplasm and nuclei in pink and purple, respectively (**Figure 6B, D**). PanINs were visualized as slightly dilated, irregularly clustered ducts with preserved structural integrity (**Figure 6B**), whereas PDAC had disorganized cell arrangement with haphazard patterns, infiltrating into the surrounding tissue with desmoplastic stroma (**Figure 6D**). Histological features found in the virtual H&E images were diagnostic factors for the discrimination of PDAC and PanIN. Virtual H&E staining of OT-TP-LSM via CycleGAN could provide comparable cellular information to conventional H&E stained histology.

Discussion

OT-TP-LSM was developed to enable rapid and precise 3D pathological examination of excised tissue specimens during both biopsy and surgery, allowing visualization of 3D cell structures. OT-TP-LSM generated a two-photon excitation light sheet using one-dimensional Bessel beam scanning, and planar images were acquired by collecting emission light from the excitation light sheet with sCMOS cameras at 400 fps maximum. Proflavine and PI were used for nuclear labeling and cell structure visualization, and intrinsic SHG contrast was used for ECM visualization. The

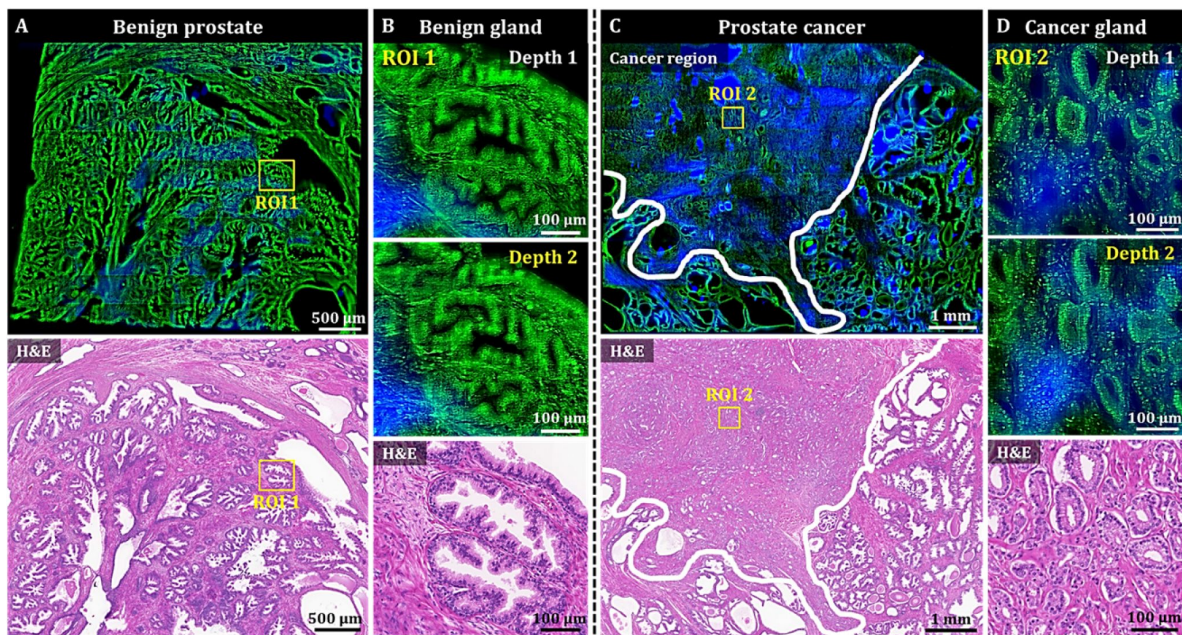


Figure 5.

3D OT-TP-LSM images of human prostate specimens: benign and adenocarcinoma

(A) Large-area OT-TP-LSM and H&E stained slide images of a benign prostate specimen. (B) Magnified two-depth OT-TP-LSM images of ROI 1 in the benign gland and a corresponding H&E image. (C) Large-area OT-TP-LSM and H&E images of a prostatic cancer specimen. A white solid line indicated the boundary between adenocarcinoma and benign regions. (D) Magnified two-depth OT-TP-LSM images of ROI 2 in adenocarcinoma glands and a corresponding H&E image. In OT-TP-LSM images, PI-labeled cells and SHG-emitting collagen were visualized in green and blue, respectively.

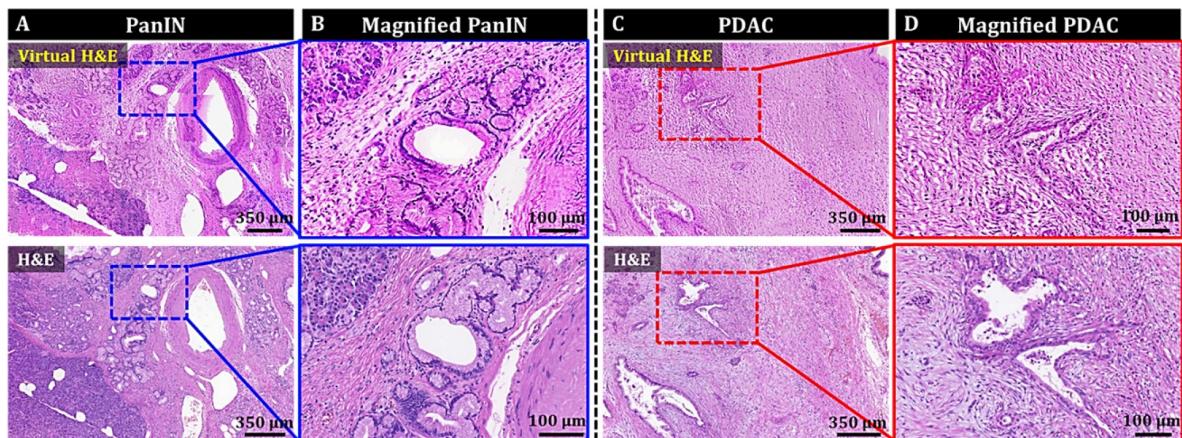


Figure 6.

Style transfer of OT-TP-LSM images for virtual H&E by cycle-consistent generational adversarial networks (CycleGAN)

(A and C) Large-area virtual H&E images and corresponding H&E stained slide images of PanIN and PDAC specimens, respectively. (B and D) Magnified virtual H&E images and corresponding H&E stained images of PanIN and PDAC, respectively.

performance of OT-TP-LSM was characterized in comparison with histopathologic images of H&E stained slides in various human cancer specimens including skin, pancreas, and prostate. 3D OT-TP-LSM images were well matched with the corresponding 2D H&E histological images with all the human tissue specimens used. The relatively high imaging depths of OT-TP-LSM enable the visualization of detailed 3D cell structures with high contrast and without distortion. The high-quality images of OT-TP-LSM may be partially attributed to the use of the nondiffractive Bessel beam for the generation of an EDOF excitation light sheet [39].

OT-TP-LSM could visualize 3D cell structures in the skin up to a depth of 60 μm by using long wavelength excitation light and proflavine labeling. Although the imaging depth was not high compared with conventional TPM, it was sufficient to visualize 3D cell structures in the skin without sectioning artifacts. The imaging depth varied depending on the tissue type, and the imaging depths of both pancreas and prostate were relatively shallow in comparison to that of the skin. This low imaging depth could be attributed to the dense cell composition and higher RI than the current immersion medium. To increase the imaging depth, PI with a relatively long emission wavelength was used. Additionally, an immersion medium with 1.5 RI could improve the imaging depth [40], and a quick optical clearing method could also be used to enhance the imaging depth [41].

We applied the unsupervised deep learning network of CycleGAN to PI-labeled OT-TP-LSM images of pancreas specimens to generate virtual H&E images, and the cytoplasm and cell nuclei, which exhibited intensity differences in greyscale, were transformed to H&E-like pseudo colors. Virtual H&E images in pancreatic cancer provided histological features equivalent to the conventional H&E. Although the CycleGAN network showed the potential for virtual H&E staining, further development is necessary to ensure robust performance and universal application. Therefore, CycleGAN will be trained using more OT-TP-LSM image data from different tissue types such as skin and prostate.

The current OT-TP-LSM has several limitations that require improvement. One issue is spherical aberration induced by the RI mismatch between the liquid prism and air when using air objective lenses in both illumination and imaging arms. Spherical aberration degraded the image resolution, particularly in the imaging arm. An immersion imaging objective lens with a high NA would be desirable to improve both image resolution and emission light collection efficiency. The excitation light sheet was generated through the rapid scanning of a single Bessel beam, resulting in a short pixel dwell time compared to that of a conventional single photon 2D light sheet. The generation of excitation light sheet with the scanning of multiple Bessel beams would increase the pixel dwell time and image contrast [42, 43]. The relatively short excitation wavelength of 770 nm was used for all the imaging to efficiently collect additional SHG light [20], but the imaging depth was limited. Longer excitation wavelengths with long emission wavelength probes would increase the imaging depth beyond those presented here.

In conclusion, OT-TP-LSM was developed for high-throughput and high-depth tissue examination. OT-TP-LSM was tested with various human cancers including skin, pancreas, and prostate by visualizing 3D cell structures. Intrinsic SHG contrast was used for visualizing ECM and detecting fibrosis. Normal glands and BCC nests were clearly distinguished, and both pancreatic and prostate cancers were clearly identified using 3D visualization of cell structures with OT-TP-LSM. Furthermore, virtual H&E staining of OT-TP-LSM using CycleGAN provided histopathologic information comparable to that from H&E stained slides. Therefore, OT-TP-LSM could be useful for rapid and precise nondestructive 3D pathology.

OT-TP-LSM setup

The schematics of OT-TP-LSM are shown in **Figure 1A**. As the light source, OT-TP-LSM used a titanium–sapphire pulse laser (Chameleon II, Coherent) with 140-fs pulse width and 80-MHz pulse repetition rate. The excitation wavelength was set at 770 nm for imaging human tissue specimens. In the illumination arm, the laser beam was expanded from 1.4 mm to 1.86 mm and then converted to a Bessel beam by using an axicon lens (131-1270 + ARB825, Eksma). The Bessel beam was relayed onto the specimen through two lens pairs of L1 (AC254-045-B, Thorlabs) and L2 (AC254-080-B, Thorlabs), and L3 (AC254-150-B, Thorlabs) and a 20× air illumination objective lens with 0.42 NA (MY20X-804, Mitutoyo). The Bessel beam diameter at the back aperture of the objective lens was approximately 6.8 mm to prevent beam clipping, and the effective illumination NA was 0.34. The excitation light sheet was generated by Y-axis scanning of the Bessel beam with a galvanometric scanner (GVS102, Thorlabs), which was positioned between L1 and L2. The liquid prism transmitted the excitation light normally through a coverslip (HSU-0101122, Marienfeld Superior), RI-matching solution, and a 0.25 mm thick round quartz window (26043, Ted Pella) at the bottom of the sample holder, and then to the sample (**Fig. 1B**). Diluted 85% glycerol (Samchun) in distilled water was used for RI-matching with the quartz window (RI: 1.45). The sample holder was connected to an x-y motorized translation stage (XY MS-2000, Applied Scientific Instrumentation) for sample translation during imaging. To remove air gaps between the quartz window of the sample holder and irregular-shaped tissue specimen, the specimen was partially immersed in the RI-matching solution and light pressure was applied on the top of the specimen. In the imaging arm, emission light was collected by the imaging objective lens (MY20X-804, Mitutoyo) through the liquid prism, spectrally separated into two channels by a dichroic mirror (T425lpxr, Chroma), and collected at two sCMOS cameras (pco-edge 4.2, PCO) after passing through a tube lens (AC254-200-A, Thorlabs), respectively. SHG light was collected in the short pass channel with an emission filter (ET376/30x, Chroma), and fluorescence was collected in the long pass channel with an emission filter (ET680SP, Chroma). Both fluorescence and SHG images were simultaneously acquired with individual gain control.

Human skin cancer specimen collection and imaging protocol

Fresh skin cancer specimens were collected under the Institutional Review Board (IRB) of Yonsei University, Severance Hospital, approved protocol (approval # 4-2021-0128). The study was conducted according to the Declaration of Helsinki Principles. OT-TP-LSM imaging was conducted within 12 h post-excision. Patient information was deidentified. Before imaging, fresh skin specimens were cut cross-sectionally to approximately 4 mm thickness and topically instilled with 400 µg/mL proflavine solution (Sigma) for 5 min, and then rinsed in phosphate-buffered saline. OT-TP-LSM imaging was conducted in 3D on the sectioned surface. After imaging, the skin specimens were fixed and processed for histopathological evaluation with H&E stained slides. Microscopic images were obtained by using a wide-field microscope (Leica Z16 APO, Leica Microsystems).

Human pancreatic and prostate cancer specimen collection and imaging protocol

Formalin-fixed, paraffin-embedded (FFPE) tissue blocks of pancreatic and prostate cancers were collected under approval (approval #, 2021-0393) from the IRB of Asan Medical Center, University of Ulsan College of Medicine. 4 µm thickness sections were made for H&E stained slides, and the remaining blocks were used for OT-TP-LSM imaging. The FFPE tissue blocks were deparaffinized with xylene (99%, Daejung) solution overnight, 1:1 xylene-100% methanol (Optima grade, Fisher scientific) mixture solution for 1 h with shaking, followed by sequentially decreasing the methanol

concentration in the xylene and methanol mixture to 90%, 80%, and 50% for 1 h each. After deparaffinization, specimens were stained with 80 µg/mL PI solution (Sigma) for 5 min, and then OT-TP-LSM imaging was conducted on the sectioned surface.

Virtual H&E staining of OT-TP-LSM via deep learning network

CycleGAN is an unsupervised deep learning network without the need for well-aligned image pairs [38]. CycleGAN was used for style transfer of OT-TP-LSM images to virtual H&E images [44–46]. CycleGAN model consisted of two generators (G: real OT-TP-LSM → fake H&E and F: real H&E → fake OT-TP-LSM), and two corresponding discriminators ($D_{\text{OT-TP-LSM}}$ and $D_{\text{H\&E}}$) to identify each fake image (Figure 6 - figure supplement 1). Cycle-consistent loss was combined with adversarial loss to prevent the well-known problem of mode collapse, where all input images mapped to the same output images [38]. For CycleGAN training, PI-labeled OT-TP-LSM and real H&E images were collected from pancreas specimens, including each of normal, premalignant lesions, and cancer. Collected images were cropped into 512 × 512 pixels patch images, and augmented by applying rotation (90°, 180°, 270°) and flip (vertical, horizontal). The total training dataset was 14,322 and 22,644 patches for OT-TP-LSM and H&E, respectively. Adam solver was used as an optimizer [47]. Hyper-parameters were set with a batch size of 1 and an initial learning rate of 0.0002 and 100 epochs. Once the training was completed, generator G was used to transform OT-TP-LSM patches into virtual H&E ones.

Acknowledgements

This work was supported in part by the National Research Foundation (NRF) grant funded by the Korea government (NRF-2020R1A2C3009309); and the Korea Medical Device Development Fund (KMDF) grant funded by the Korean government (Project Number: 9991006749, KMDF_PR_20200901_0076).

Conflict of interest statements

No conflicts of interest were declared.

Supplementary figure legends

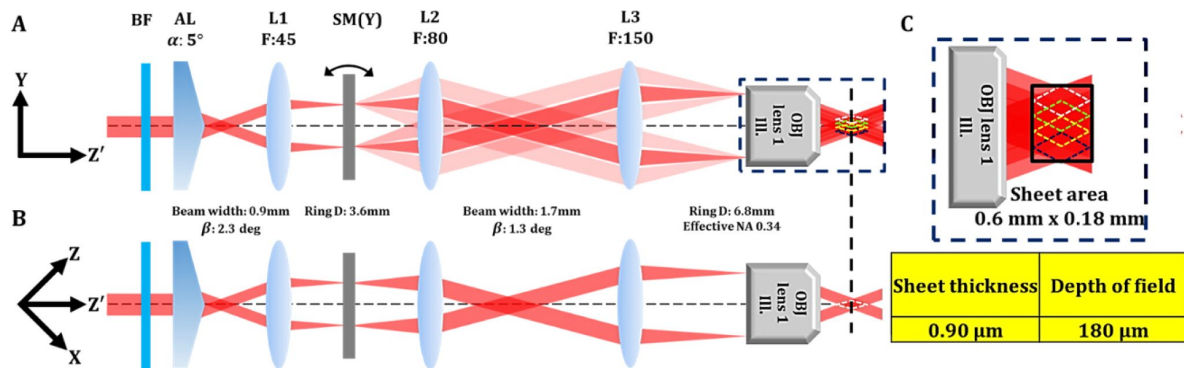


Figure 1 - figure supplement 1.

Detail optical configuration of illumination arm in open-top two-photon light sheet microscopy (OT-TP-LSM)

(A) Illustration of beam path at Y-Z' plan. L: lens, BF: barrier filter, AL: axicon lens, SM: scanning mirror, Obj: objective lens. Two-photon light sheet with extended depth of field (DOF) was generated by scanning a Bessel beam in the Y-axis direction rapidly. (B) Illustration of beam path at Z-X plan. (C) Magnified image and designed dimension of the Bessel beam based light sheet. The excitation light sheet was designed to have a DOF of 180 μm with a thickness of 0.9 μm .

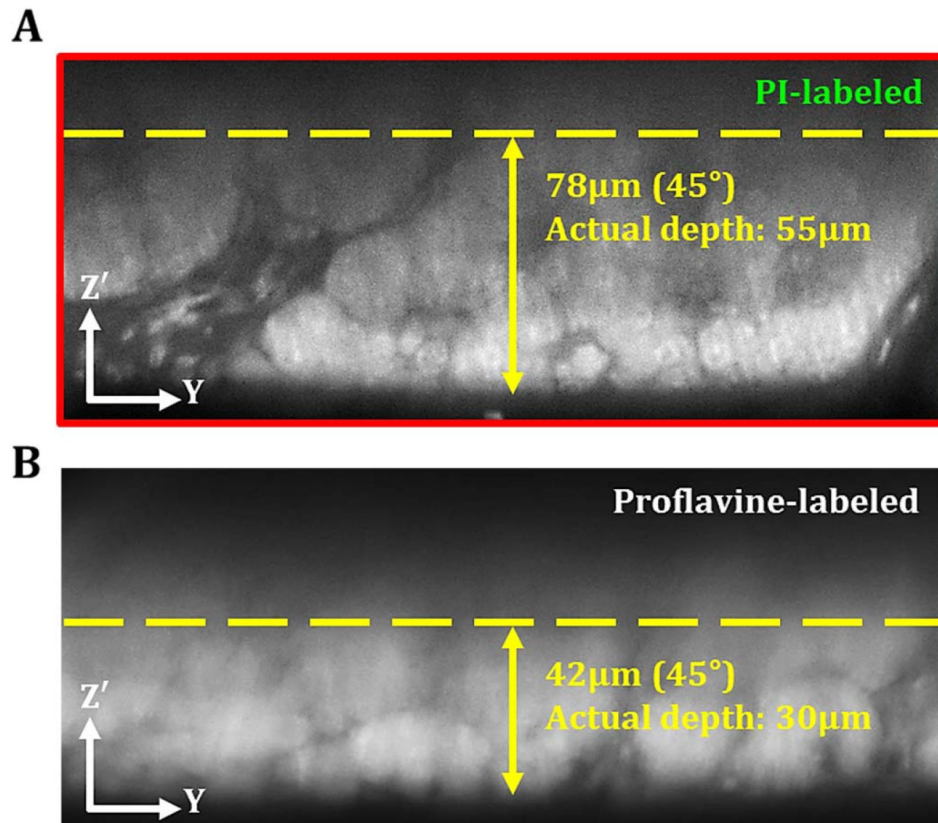


Figure 3 - figure supplement 1.

Comparison of imaging depth between propidium iodide (PI) and proflavine in human pancreas

(A) 45° oblique OT-TP-LSM image of pancreas specimens after PI cell labeling. (B) 45° oblique OT-TP-LSM image of pancreas specimens after proflavine cell labeling. PI labeling enabled the deeper imaging up to approximately 55 μm from the surface owing to its relatively long peak emission wavelength compared to proflavine. Both pancreas specimens were incubated with PI and proflavine for 5 mins, respectively.

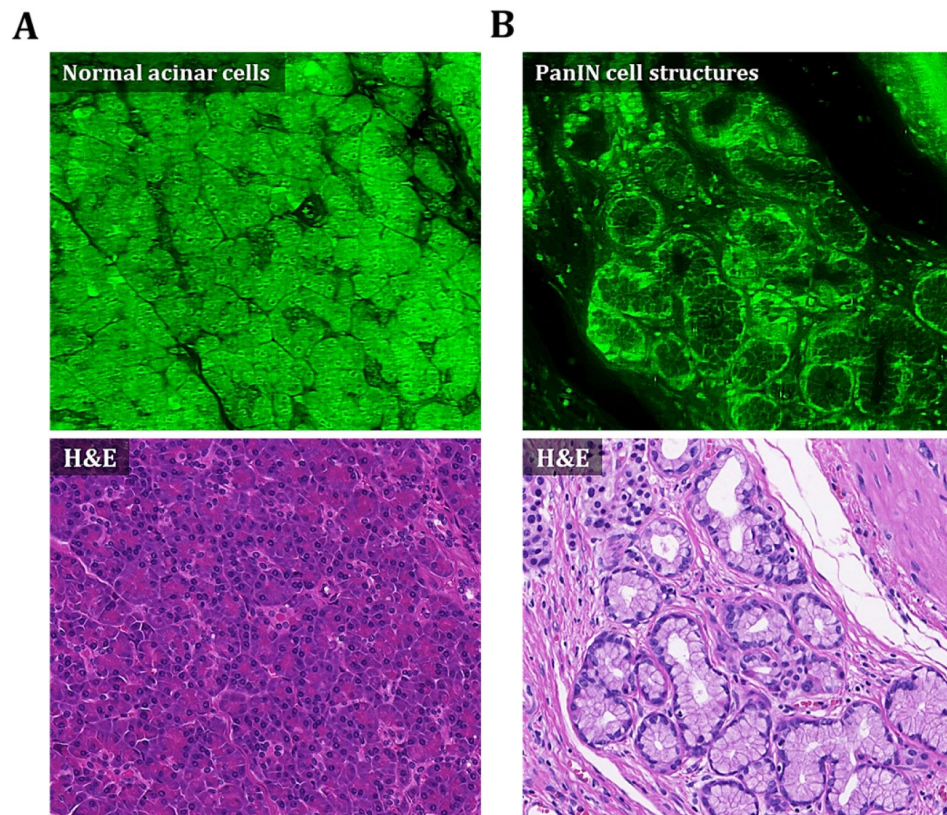


Figure 3 - figure supplement 2.

PI cell staining characteristics in human pancreas

(A) OT-TP-LSM image of acinar cell structures in normal pancreas specimens after PI cell labeling and corresponding H&E image. (B) OT-TP-LSM image of pancreatic intraepithelial neoplasia (PanIN) structures in premalignant pancreas after PI cell labeling and corresponding H&E image. In OT-TP-LSM images, PI fluorescence was displayed in green color. PI showed nuclear and cytoplasmic labeling properties of cells in both acini and neoplastic structures. Cell nuclei were identified with relatively strong and weak fluorescence in the membrane and core, respectively.

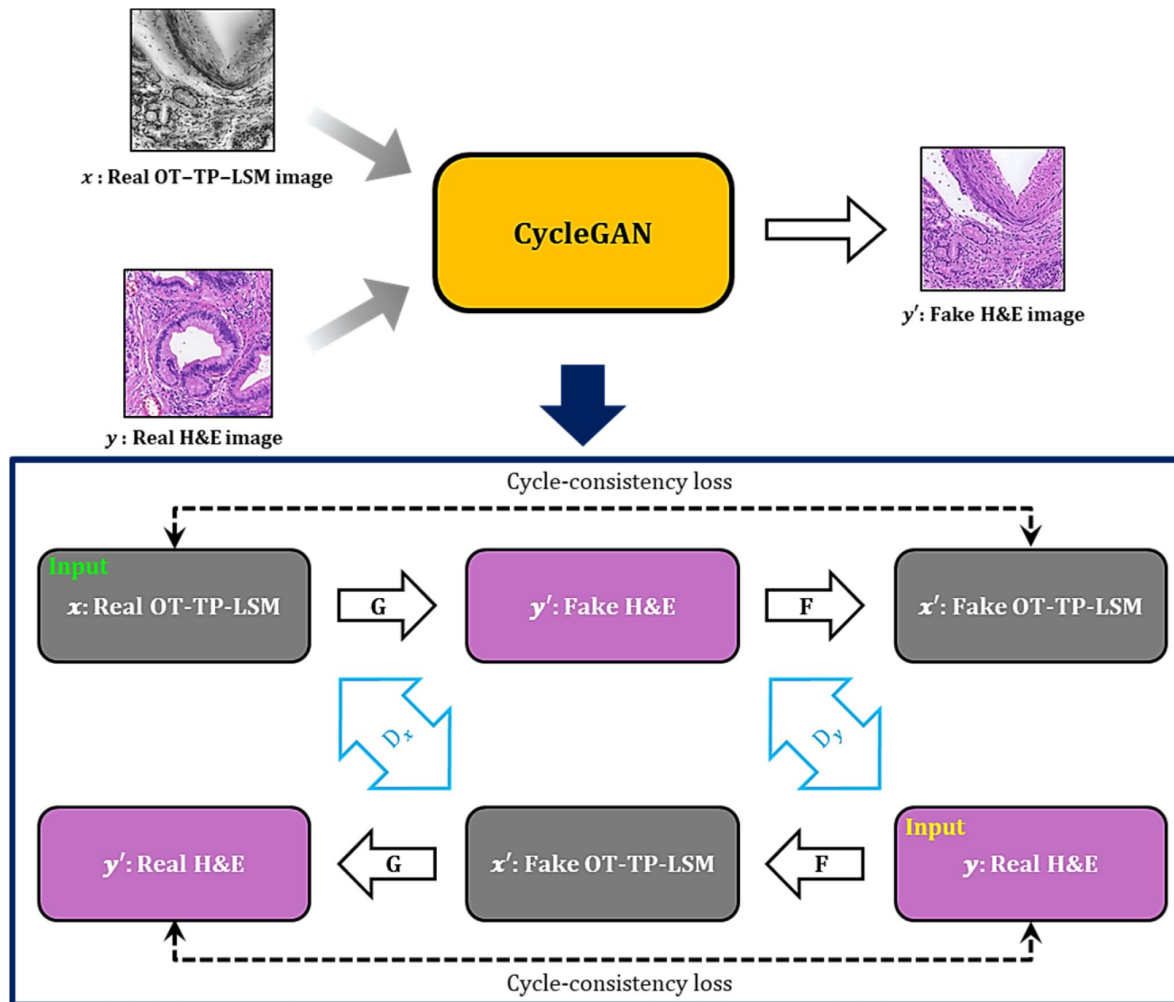


Figure 6 - figure supplement 1.

Cycle-consistent generational adversarial networks (CycleGAN) workflow for style transfer of OT-TP-LSM image to virtual hematoxylin and eosin (H&E) image

Real OT-TP-LSM image and real H&E image were assigned as x and y , and the corresponding fake image is additionally marked with a prime. The generator G transformed the real OT-TP-LSM image into a fake virtual H&E-stained image. Generator F transformed the real H&E image into a fake OT-TP-LSM image. The discriminator D_x classifies real OT-TP-LSM image x and fake OT-TP-LSM image x' . The discriminator D_y classifies real H&E image y and fake virtual H&E image y' . Both Cycle-consistent loss and adversarial loss were used as the loss function, which was to guarantee the performance of inverse transform from G and F by preserving the morphological features of real images.

Video legend

Video 1. Three-dimensional (3D) visualization of basal cell carcinoma (BCC) structures and normal cell structures.

References

1. Liu JTC, Glaser AK, Bera K, et al. (2021) **Harnessing non-destructive 3D pathology** *Nat Biomed Eng* **5**:203–218
2. Almagro J, Messal HA, Thin MZ, et al. (2021) **Tissue clearing to examine tumour complexity in three dimensions** *Nat Rev Cancer* **21**:718–730
3. Bishop KW, Maitland KC, Rajadhyaksha M, et al. (2022) **In vivo microscopy as an adjunctive tool to guide detection, diagnosis, and treatment** *J Biomed Opt* **27**
4. Serafin R, Koyuncu C, Xie W, et al. (2023) **Nondestructive 3D pathology with analysis of nuclear features for prostate cancer risk assessment** *J Pathol* **260**:390–401
5. Filler TJ, Peuker ET (2000) **Reflection contrast microscopy (RCM): a forgotten technique?** *J Pathol* **190**:635–638
6. van Royen ME, Verhoef EI, Kweldam CF, et al. (2016) **Three-dimensional microscopic analysis of clinical prostate specimens** *Histopathology* **69**:985–992
7. Verhoef EI, van Cappellen WA, Slotman JA, et al. (2019) **Three-dimensional analysis reveals two major architectural subgroups of prostate cancer growth patterns** *Modern Pathol* **32**:1032–1041
8. Yoshitake T, Giacomelli MG, Cahill LC, et al. (2016) **Direct comparison between confocal and multiphoton microscopy for rapid histopathological evaluation of unfixed human breast tissue** *J Biomed Opt* **21**
9. Tao YK, Shen DJ, Sheikine Y, et al. (2014) **Assessment of breast pathologies using nonlinear microscopy** *P Natl Acad Sci USA* **111**:15304–15309
10. Baugh LM, Liu ZY, Quinn KP, et al. (2017) **Non-destructive two-photon excited fluorescence imaging identifies early nodules in calcific aortic-valve disease** *Nature Biomedical Engineering* **1**:914–924
11. Patel KB, Liang WX, Casper MJ, et al. (2022) **High-speed light-sheet microscopy for the in-situ acquisition of volumetric histological images of living tissue** *Nature Biomedical Engineering* **6**:569–583
12. Voleti V, Patel KB, Li WZ, et al. (2019) **Real-time volumetric microscopy of in vivo dynamics and large-scale samples with SCAPE 2.0** *Nat Methods* **16**:1054–1062
13. McGorty R, Liu H, Kamiyama D, et al. (2015) **Open-top selective plane illumination microscope for conventionally mounted specimens** *Opt Express* **23**:16142–16153
14. Glaser AK, Reder NP, Chen Y, et al. (2017) **Light-sheet microscopy for slide-free non-destructive pathology of large clinical specimens** *Nature Biomedical Engineering* **1**
15. Glaser AK, Bishop KW, Barner LA, et al. (2022) **A hybrid open-top light-sheet microscope for versatile multi-scale imaging of cleared tissues** *Nat Methods* **19**:613–619

16. Gao G, Miyasato D, Barner LA, et al. (2023) **Comprehensive Surface Histology of Fresh Resection Margins With Rapid Open-Top Light-Sheet (OTLS) Microscopy** *Ieee T Bio-Med Eng* **70**:2160–2171
17. Denk W, Strickler JH, Webb WW (1990) **Two-photon laser scanning fluorescence microscopy** *Science* **248**:73–76
18. So PTC, Dong CY, Masters BR, et al. (2000) **Two-photon excitation fluorescence microscopy** *Annu Rev Biomed Eng* **2**:399–429
19. Helmchen F, Denk W (2005) **Deep tissue two-photon microscopy** *Nat Methods* **2**:932–940
20. Zipfel WR, Williams RM, Christie R, et al. (2003) **Live tissue intrinsic emission microscopy using multiphoton-excited native fluorescence and second harmonic generation** *Proc Natl Acad Sci U S A* **100**:7075–7080
21. Fast A, Lal A, Durkin AF, et al. (2020) **Fast, large area multiphoton exoscope (FLAME) for macroscopic imaging with microscopic resolution of human skin** *Sci Rep* **10**
22. Park WY, Kim B, Chun JH, et al. (2022) **High-contrast visualization of human skin cancers with combined reflectance confocal and moxifloxacin-based two-photon microscopy: An ex vivo study** *Lasers Surg Med* **54**:1226–1237
23. Fahrbach FO, Gurchenkov V, Alessandri K, et al. (2013) **Light-sheet microscopy in thick media using scanned Bessel beams and two-photon fluorescence excitation** *Opt Express* **21**:13824–13839
24. Mahou P, Vermot J, Beaupaire E, et al. (2014) **Multicolor two-photon light-sheet microscopy** *Nat Methods* **11**:600–601
25. Wolf S, Supatto W, Debregeas G, et al. (2015) **Whole-brain functional imaging with two-photon light-sheet microscopy** *Nat Methods* **12**:379–380
26. Maioli V, Boniface A, Mahou P, et al. (2020) **Fast in vivo multiphoton light-sheet microscopy with optimal pulse frequency** *Biomed Opt Express* **11**:6012–6026
27. de Vito G, Turrini L, Mullenbroich C, et al. (2022) **Fast whole-brain imaging of seizures in zebrafish larvae by two-photon light-sheet microscopy** *Biomed Opt Express* **13**:1516–1536
28. Planchon TA, Gao L, Milkie DE, et al. (2011) **Rapid three-dimensional isotropic imaging of living cells using Bessel beam plane illumination** *Nat Methods* **8**:417–423
29. Fan JL, Rivera JA, Sun W, et al. (2020) **High-speed volumetric two-photon fluorescence imaging of neurovascular dynamics** *Nat Commun* **11**
30. Rieger AM, Hall BE, Le TL, et al. (2010) **Conventional apoptosis assays using propidium iodide generate a significant number of false positives that prevent accurate assessment of cell death** *J Immunol Methods* **358**:81–92
31. Niu JF, Li CM, Wu HH, et al. (2015) **Propidium iodide (PI) stains Nissl bodies and may serve as a quick marker for total neuronal cell count** *Acta Histochem* **117**:182–187
32. Lemaire K, Chimienti F, Schuit F (2012) **Zinc transporters and their role in the pancreatic β -cell** *Journal of Diabetes Investigation* **3**:202–211

33. Hruban RH, Adsay NV, Albores-Saavedra J, et al. (2001) **Pancreatic intraepithelial neoplasia: a new nomenclature and classification system for pancreatic duct lesions** *Am J Surg Pathol* **25**:579–586
34. McGinnis T, Bantis LE, Madan R, et al. (2020) **Survival Outcomes of Pancreatic Intraepithelial Neoplasm (PanIN) versus Intraductal Papillary Mucinous Neoplasm (IPMN) Associated Pancreatic Adenocarcinoma** *J Clin Med* **9**
35. Adsay NV, Bandyopadhyay S, Basturk O, et al. (2004) **Chronic pancreatitis or pancreatic ductal adenocarcinoma?** *Semin Diagn Pathol* **21**:268–276
36. Drifka CR, Tod J, Loeffler AG, et al. (2015) **Periductal stromal collagen topology of pancreatic ductal adenocarcinoma differs from that of normal and chronic pancreatitis** *Modern Pathol* **28**:1470–1480
37. Ray A, Callaway MK, Rodriguez-Merced NJ, et al. (2022) **Stromal architecture directs early dissemination in pancreatic ductal adenocarcinoma** *JCI Insight* **7**
38. Zhu JY, Park T, Isola P, et al. (2017) **Unpaired Image-to-Image Translation using Cycle-Consistent Adversarial Networks** *Ieee I Conf Comp Vis* :2242–2251
39. Olarte OE, Licea-Rodriguez J, Palero JA, et al. (2012) **Image formation by linear and nonlinear digital scanned light-sheet fluorescence microscopy with Gaussian and Bessel beam profiles** *Biomed Opt Express* **3**:1492–1505
40. Young PA, Clendenon SG, Byars JM, et al. (2011) **The effects of refractive index heterogeneity within kidney tissue on multiphoton fluorescence excitation microscopy** *J Microsc-Oxford* **242**:148–156
41. Aoyagi Y, Kawakami R, Osanai H, et al. (2015) **A Rapid Optical Clearing Protocol Using 2,2'-Thiodiethanol for Microscopic Observation of Fixed Mouse Brain** *Plos One* **10**
42. Minamikawa T, Hashimoto M, Fujita K, et al. (2009) **Multi-focus excitation coherent anti-Stokes Raman scattering (CARS) microscopy and its applications for real-time imaging** *Opt Express* **17**:9526–9536
43. Chen X, Zong W, Li R, et al. (2016) **Two-photon light-sheet nanoscopy by fluorescence fluctuation correlation analysis** *Nanoscale* **8**:9982–9987
44. Chen Z, Yu W, Wong IHM, et al. (2021) **Deep-learning-assisted microscopy with ultraviolet surface excitation for rapid slide-free histological imaging** *Biomed Opt Express* **12**:5920–5938
45. Cao R, Nelson SD, Davis S, et al. (2023) **Label-free intraoperative histology of bone tissue via deep-learning-assisted ultraviolet photoacoustic microscopy** *Nat Biomed Eng* **7**:124–134
46. Abraham T, Shaw A, O'Connor D, et al. (2020) **Slide-free MUSE microscopy to H&E histology modality conversion via unpaired image-to-image translation GAN Models**
47. Kingma DP, Ba J. (2014) **Adam: A method for stochastic optimization**

Article and author information

Won Yeong Park

Department of Mechanical Engineering, Pohang University of Science and Technology, Pohang, Gyeongsangbuk, 37673, Republic of Korea

Jieun Yun

Department of Mechanical Engineering, Pohang University of Science and Technology, Pohang, Gyeongsangbuk, 37673, Republic of Korea

Jinho Shin

Department of Medicine, University of Ulsan College of Medicine, Seoul, 05505, Republic of Korea

Byung Ho Oh

Department of Dermatology, College of Medicine, Yonsei University, Seoul, 03722, Republic of Korea

Gilsuk Yoon

Department of Pathology, School of Medicine, Kyungpook National University, Daegu, 41944, Republic of Korea

Seung-Mo Hong

Department of Pathology, Asan Medical Center, University of Ulsan College of Medicine, Seoul, 05505, Republic of Korea

Ki Hean Kim

Department of Mechanical Engineering, Pohang University of Science and Technology, Pohang, Gyeongsangbuk, 37673, Republic of Korea, Department of I-Bio, Pohang University of Science and Technology, Pohang, Gyeongsangbuk, 37673, Republic of Korea

For correspondence: kiheankim@postech.ac.kr

ORCID iD: [0000-0003-3410-7706](https://orcid.org/0000-0003-3410-7706)

Copyright

© 2023, Park et al.

This article is distributed under the terms of the [Creative Commons Attribution License](https://creativecommons.org/licenses/by/4.0/), which permits unrestricted use and redistribution provided that the original author and source are credited.

Editors

Reviewing Editor

Vitaly Ryu

Icahn School of Medicine at Mount Sinai, United States of America

Senior Editor

Diane Harper

University of Michigan, United States of America

Reviewer #1 (Public Review):**Summary:**

This manuscript presents the development of a new microscope method termed "open-top two-photon light sheet microscopy (OT-TP-LSM)". While the key aspects of the new approach (open-top LSM and Two-photon microscopy) have been demonstrated separately, this is the first system of integrating the two. The integration provides better imaging depth than a single-photon excitation OT-LSM.

Strengths:

- The use of liquid prism to minimize the aberration induced by index mismatching is interesting and potentially helpful to other researchers in the field.
- The use of propidium iodide (PI) provided a deeper imaging depth.

Weaknesses:

- Details are lacking on imaging time, data size, the processing time to generate large-area en face images, and inference time to generate pseudo H&E images. This makes it difficult to assess how applicable the new microscope approach might be in various pathology applications.

Reviewer #2 (Public Review):**Summary:**

In this manuscript, the authors developed an open-top two-photon light sheet microscopy (OT-TP-LSM) that enables high-throughput and high-depth investigation of 3D cell structures. The data presented here shows that OT-T-LSM could be a complementary technique to traditional imaging workflows of human cancer cells.

Strengths:

High-speed and high-depth imaging of human cells in an open-top configuration is the main strength of the presented study. An extended depth of field of 180 μm in 0.9 μm thickness was achieved together with an acquisition of 0.24 mm^2/s . This was confirmed by 3D visualization of human cancer cells in the skin, pancreas, and prostate.

Weaknesses:

The complementary aspect of the presented technique in human pathological samples is not convincingly presented. The traditional hematoxylin and eosin (H&E) staining is a well-established and widely used technique to detect human cancer cells. What would be the benefit of 3D cell visualization in an OT-TP-LSM microscope for cancer detection in addition to H&E staining?